

Figure 1 (Prior Art)

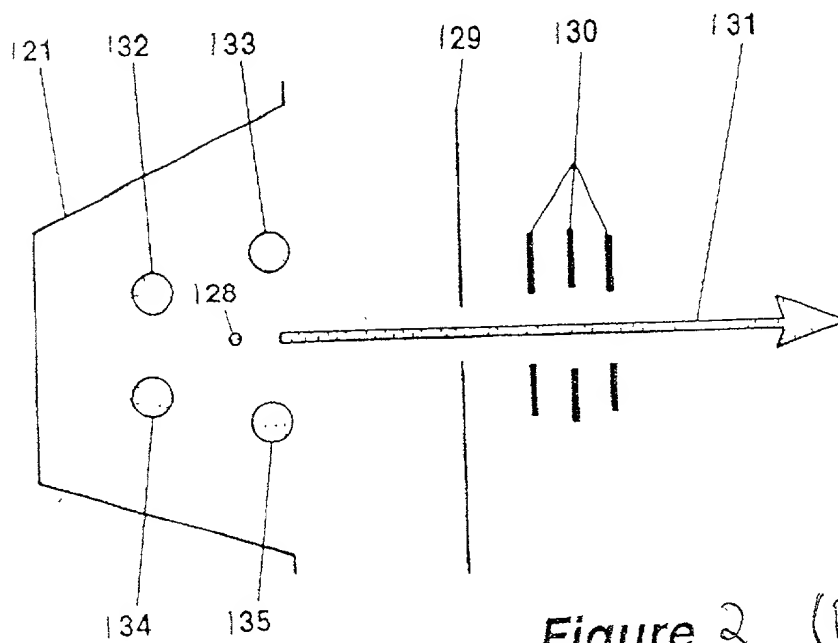


Figure 2 (Prior Art)

32 ↓

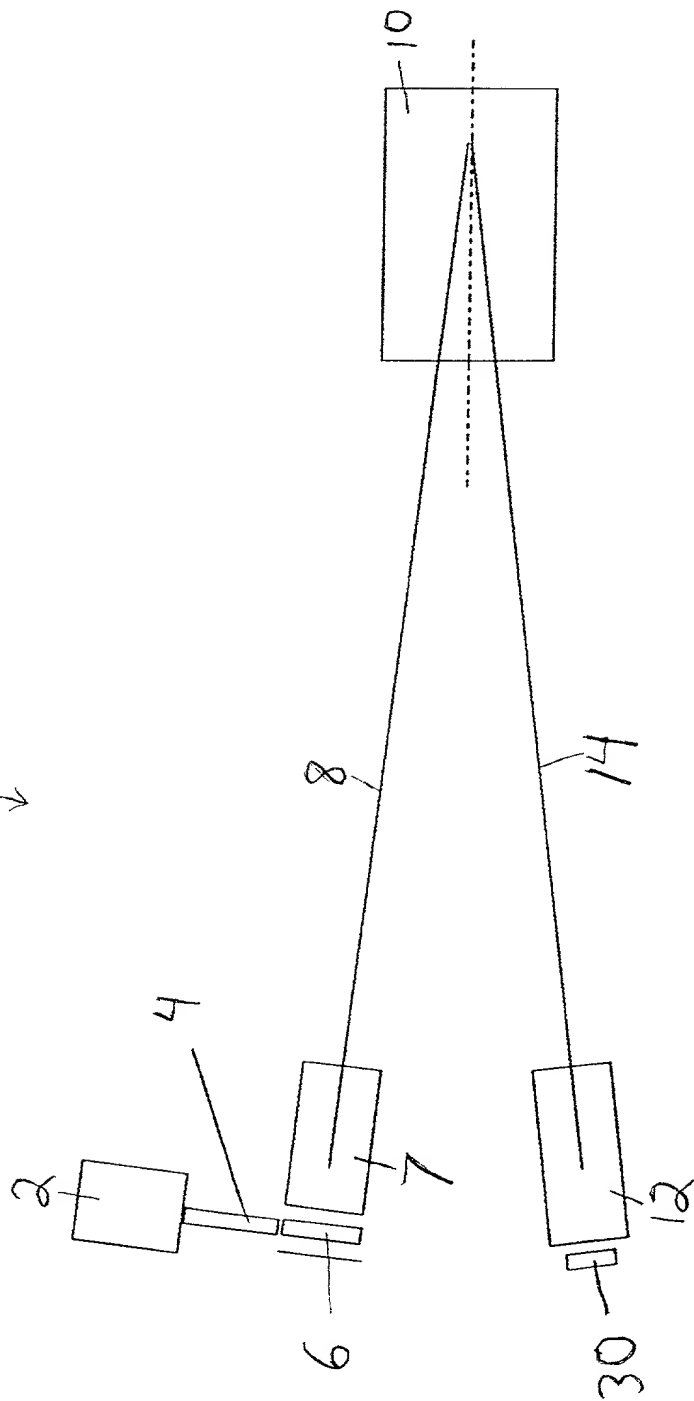


Figure 3

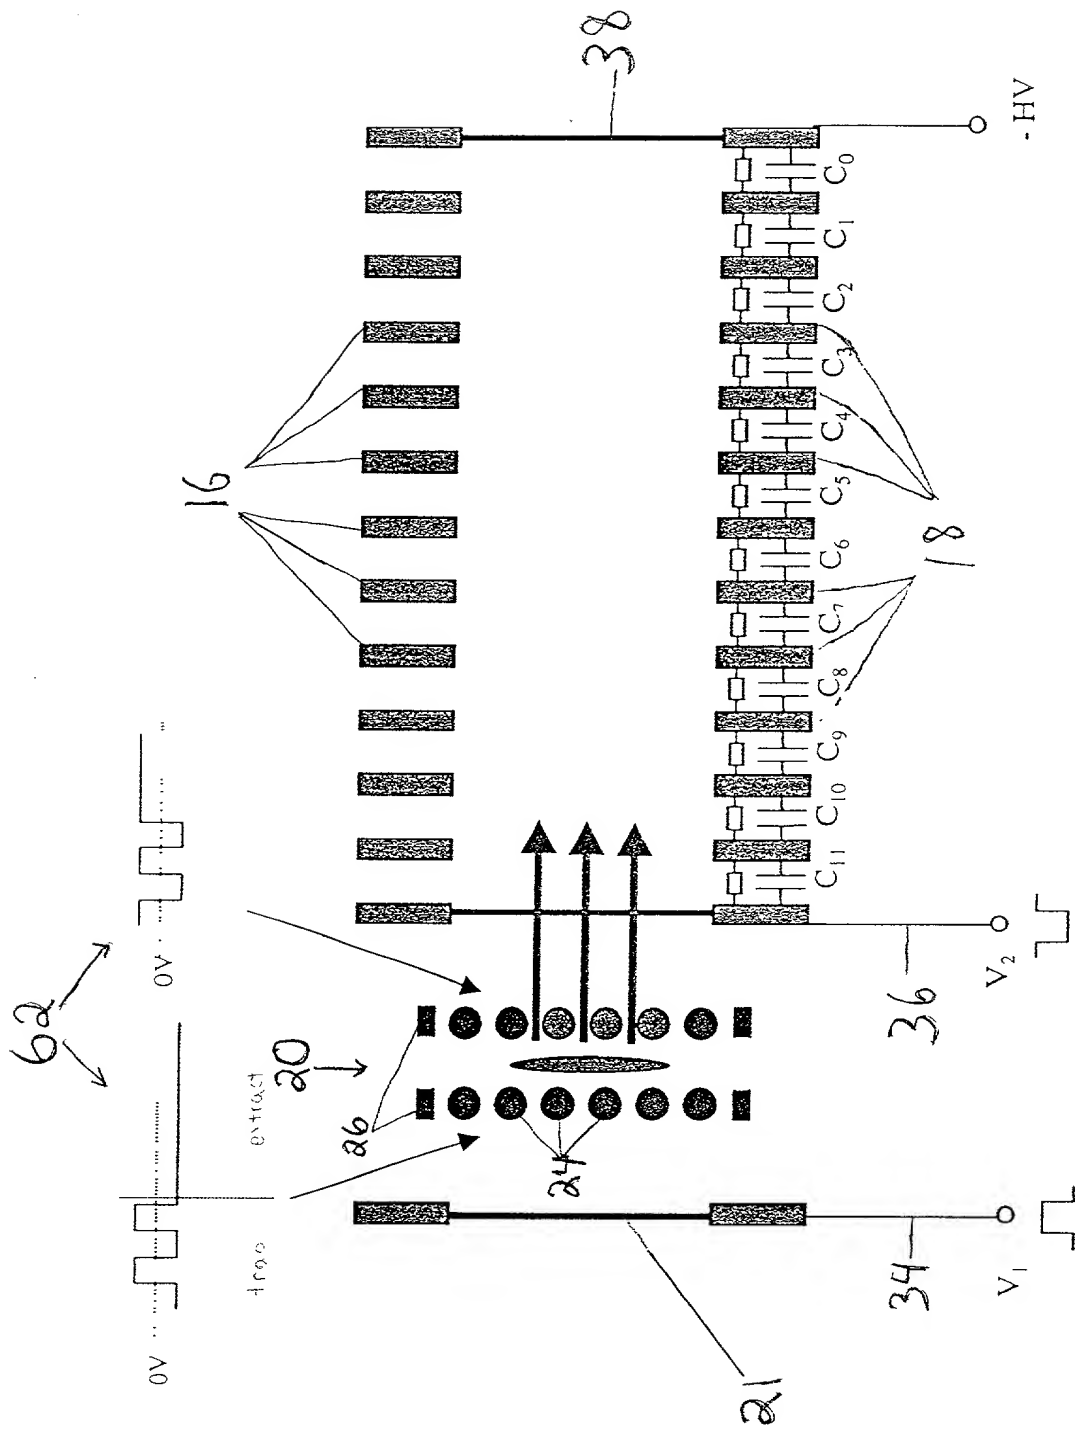


Figure 4

20

24



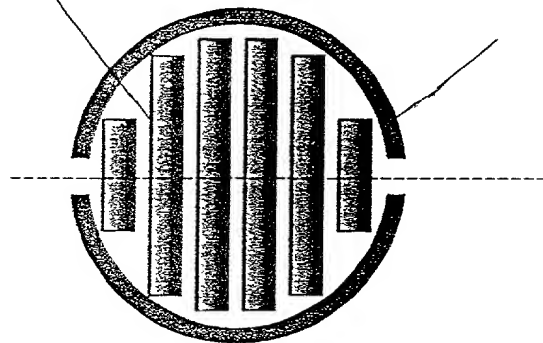


Figure 5A

28

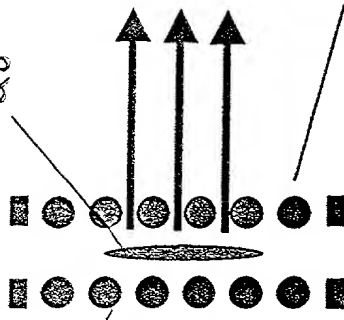

63



0V




Figure 5B

52

22 ↓

26 20

42

40

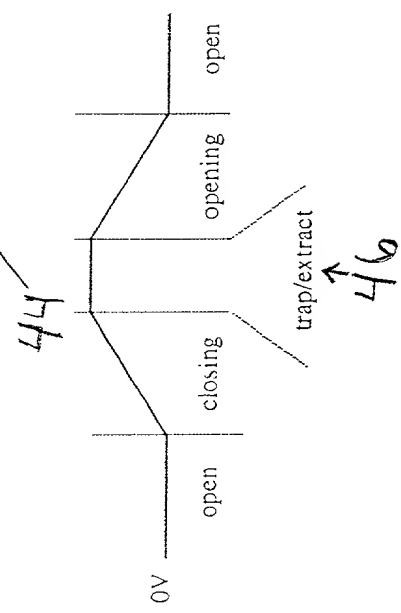
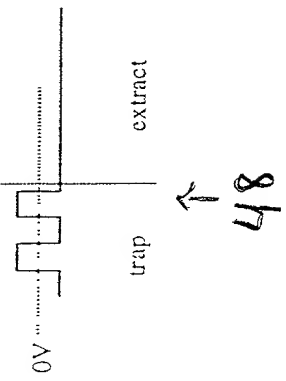


Figure 6

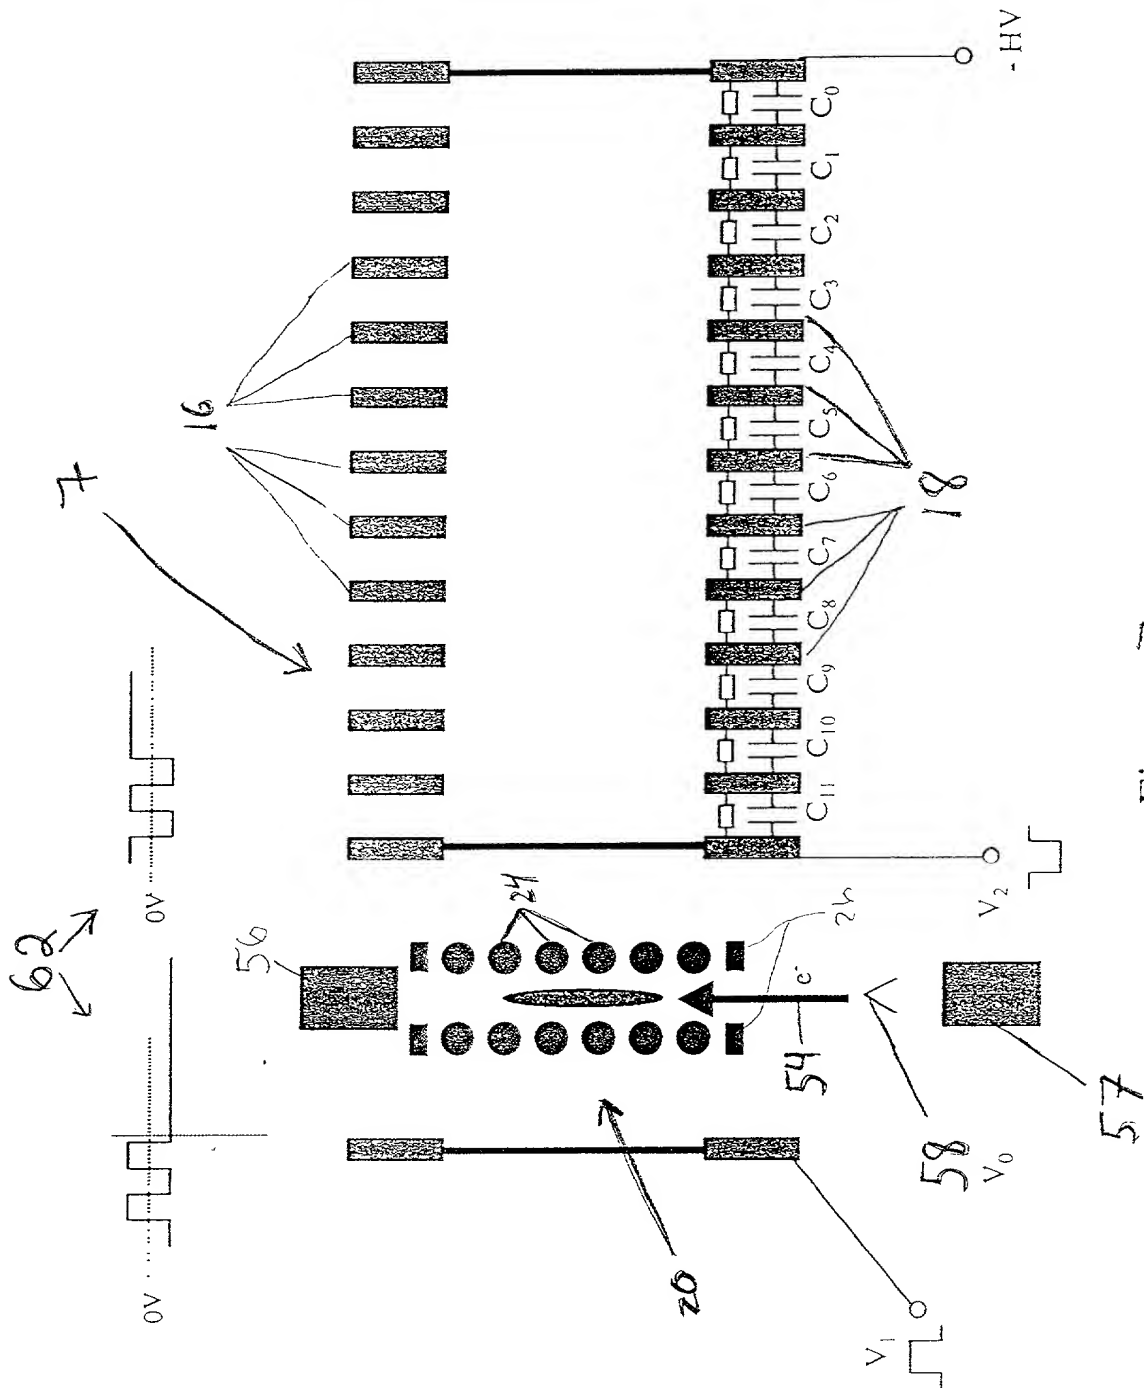


Figure 7

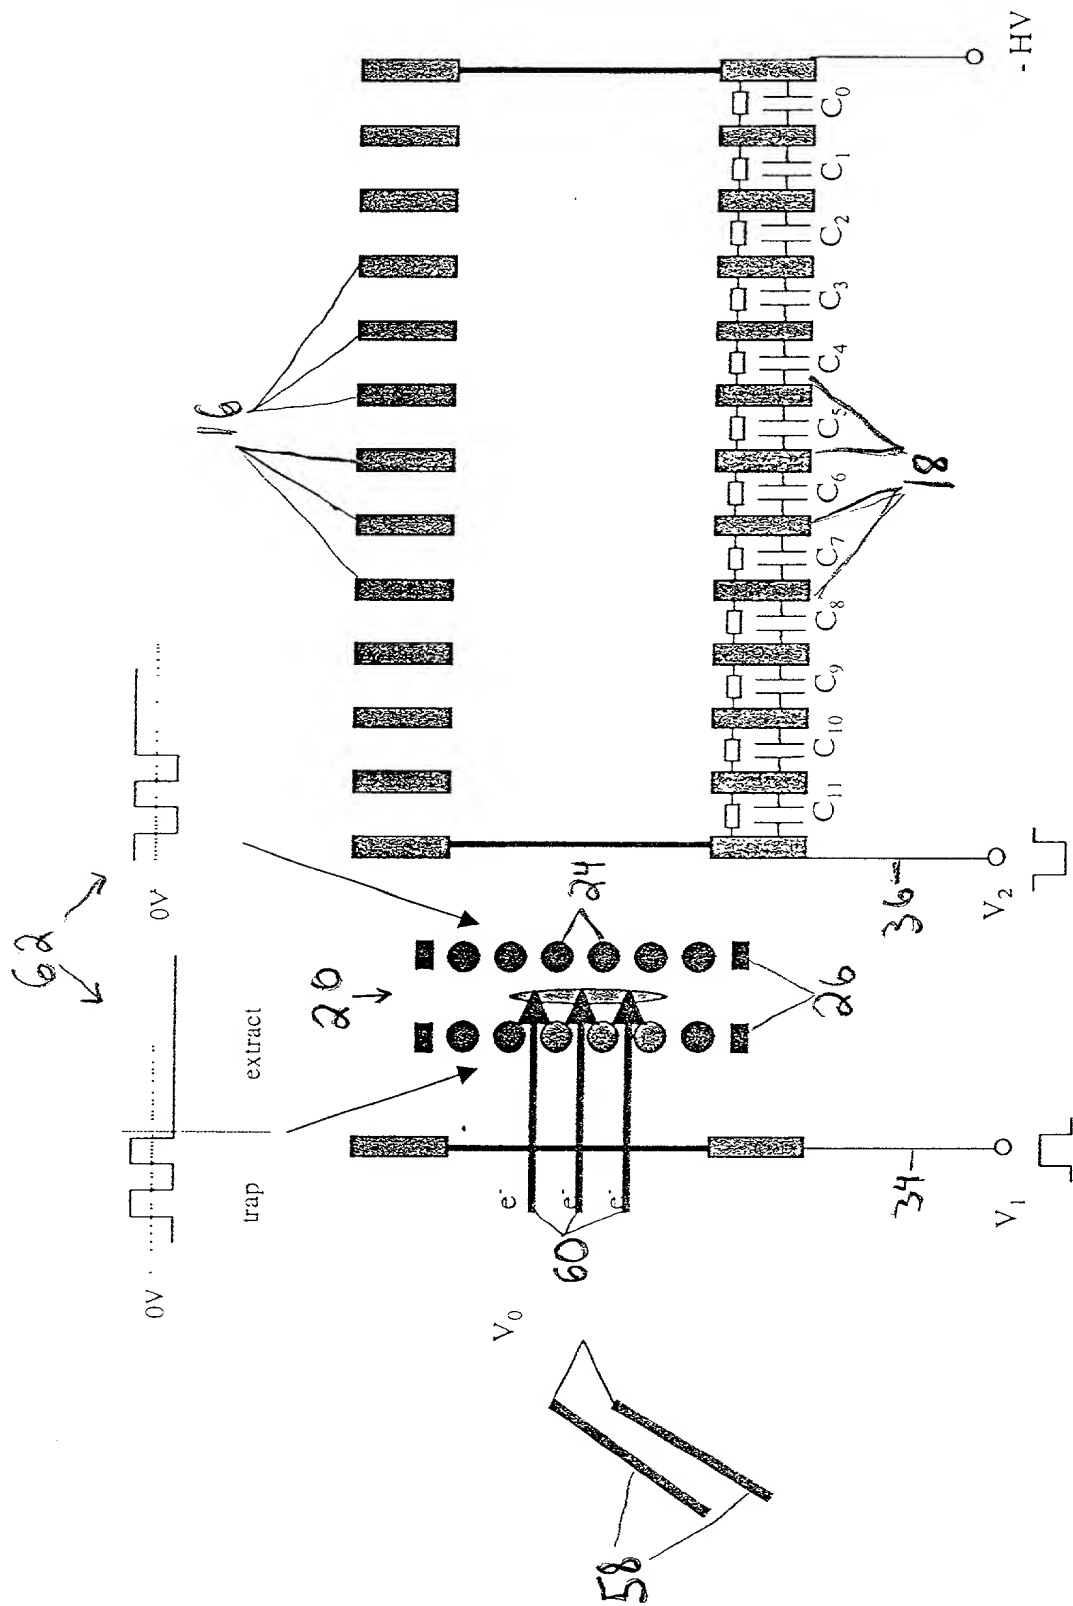


Figure 8

TOP-TECH

angio li gate open 300 us

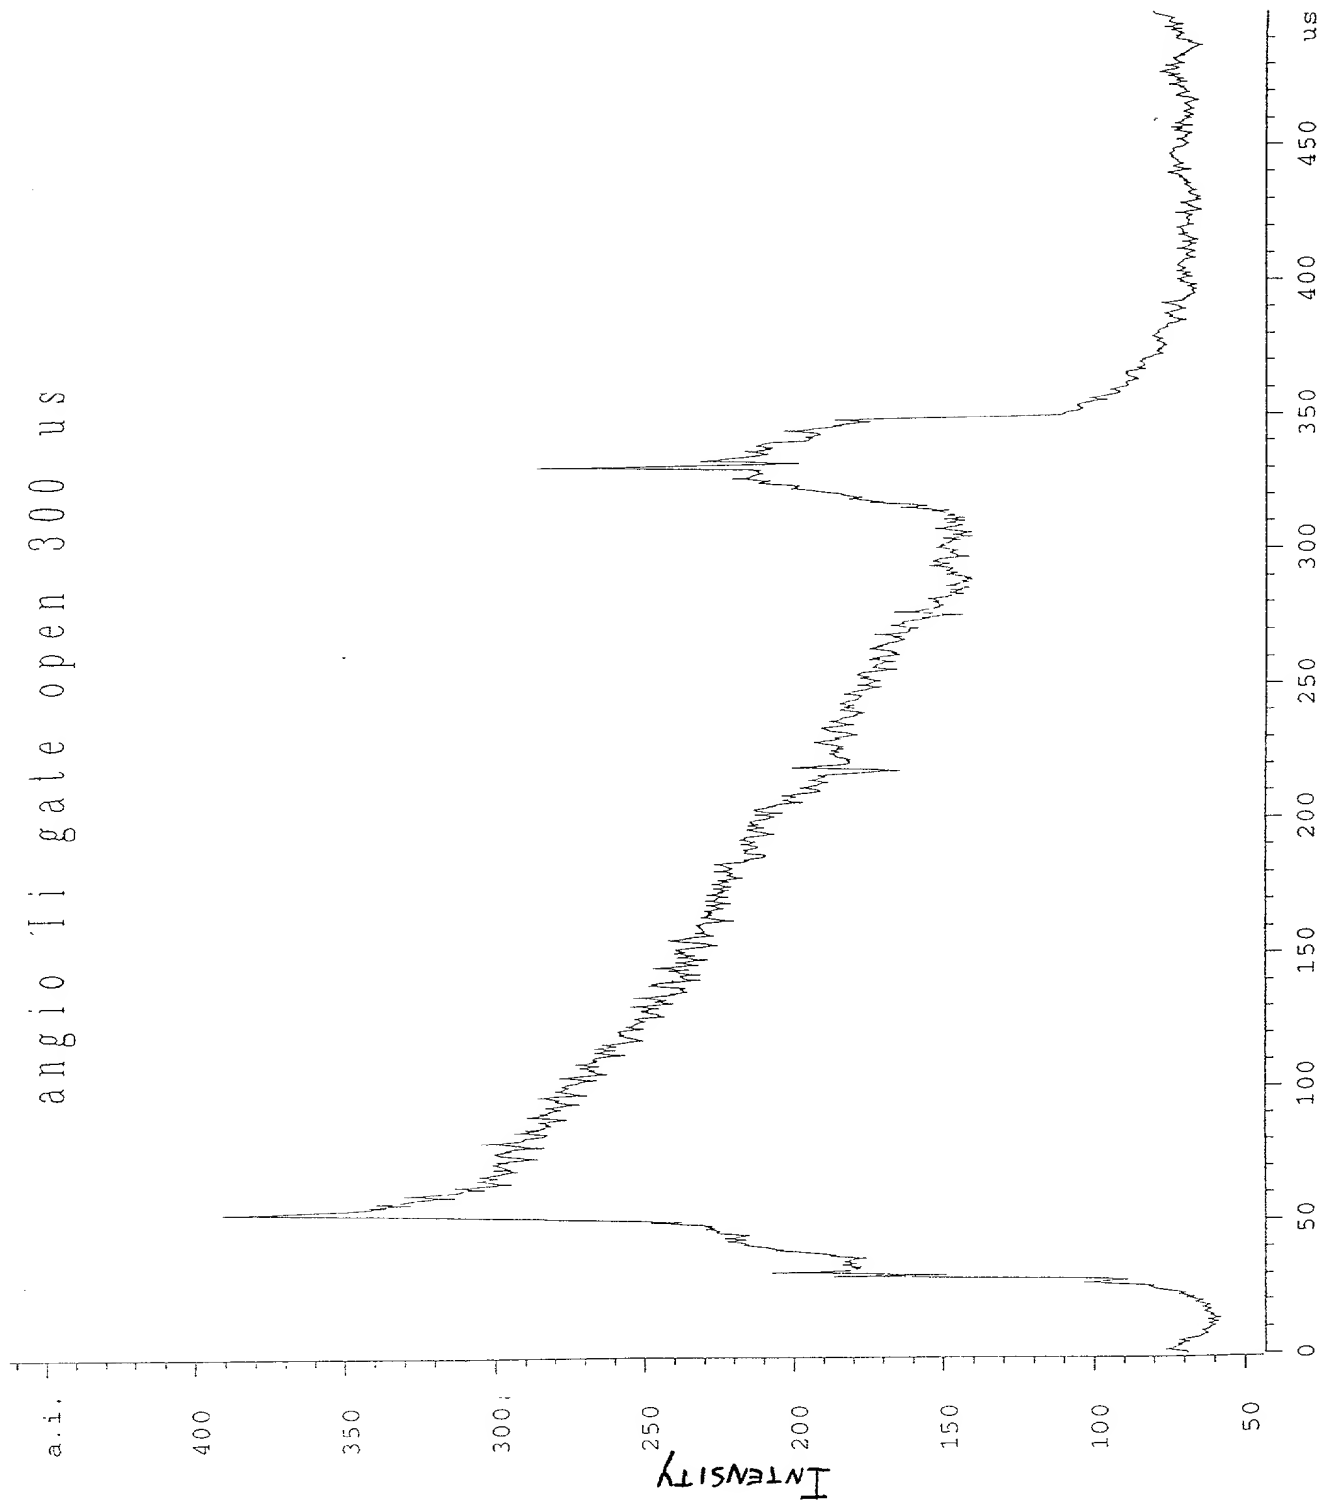


FIGURE 9

PULSE DURATION - MICROSECONDS